

Using Tunable Filter Spectroscopy for Compositional Gas Measurement in the Drilling Industry

Fiona Mueller-Thode

Pason System Corp.

Sales@pason.com

6130 – 3rd Street SE Calgary, Alberta T2H 1K4

Summary

The oil and gas industry has seen a rapid increase in horizontal drilling and the corresponding need for reliable formation data to make steering decisions. Additionally, finding Natural Gas Liquids (NGLs) and properly completing a well have become more critical to making a gas well economical. These processes become easier when compositional gas data is available.

Introduction

Total gas detectors commonly used in Canada provide a real-time gas trace, but fail to provide compositional information of the hydrocarbons in the formation. This compositional information can be useful when making drilling and completion decisions. Gas chromatographs provide an accurate composition, but are limited in that they require additional technical staff onsite and have a very low data frequency. Due to the associated costs, the use of Gas Chromatographs has virtually disappeared from use in Canada. Curiously, they are still widely used in the US.

A revolutionary new technology utilizing tunable filter spectroscopy allows the collection of real-time, accurate compositional gas data without additional technicians on location. This technology enables the development of instruments that deliver the best of both worlds; real time compositional gas data in a rugged unmanned solution. This eliminates the need for complicated, expensive and temperamental gas chromatographs, while replacing the total gas detectors that are currently the industry standard.

Theory

Through the use of tunable filter spectroscopy compositional data is collected. Early field tested prototypes are able to analyze the breakdown of gas readings including methane, ethane, propane, butane, isobutane, and CO₂, with a remarkably higher frequency than gas chromatographs are able to analyze. The technology can be expanded to include the measurement of pentanes.

The compositional data collected with this technology forms the basis for plots of the wetness, balance, and character ratios. These ratios are critical geological indicators used to define the oil/gas and oil/water contact points and detect the presence of natural gas liquids in the formation. This data can be used to infer geological properties of the formation being drilled and thus make better steering, drilling, and completion decisions.


The figure below shows how to interpret these ratios.

Balance Ratio	Wetness Ratio	Reservoir Fluid and Production Potential
> 100		Very light, dry gas Typically non-associated and non-productive such as the occurrence of high pressured methane, metagenic cracking below the oil window, bacterial methane etc
< 100	< 0.5	Possible production of light, dry gas
Wh < Bh < 100	0.5 – 17.5	Productive gas, increasing in wetness as the curves are closer together
< Wh	0.5 – 17.5	Productive, very wet gas or condensate or high gravity oil with high GOR (Bh<Wh indicates liquid, but Wh still indicates gas)
< Wh	17.5 – 40	Productive oil with decreasing gravity as the curve separation increases
<< Wh	17.5 – 40	Lower production potential of low gravity, low gas saturation oil
	> 40	Very low gravity or residual oil

Figure 1: Interpreting Balance and Wetness Ratios.

Examples

The chart below shows an example of how wetness and balance ratios can be used to infer fluid contact points and to make informed steering decisions.

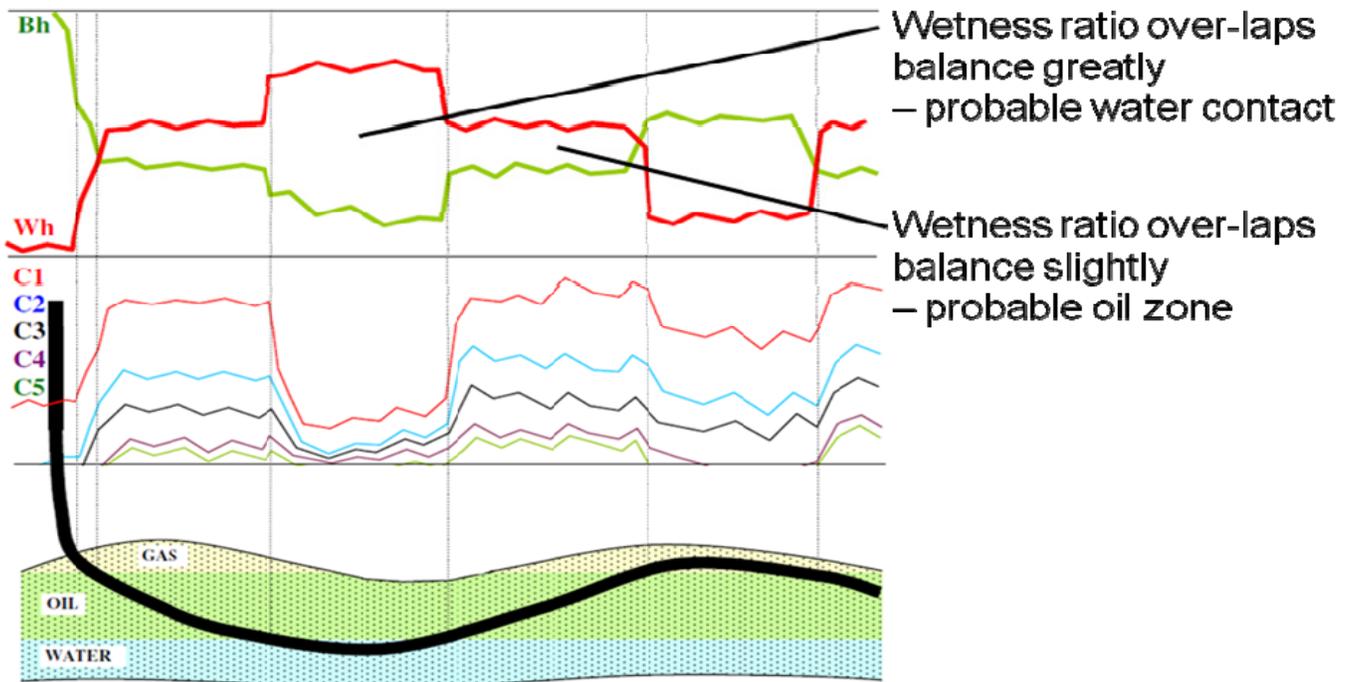

Fluid contact identification and course of correction

Figure 2: Using Wetness and Balance ratios for geo-steering applications.

Conclusions

The use of compositional gas data in the drilling industry can be a very useful and profitable tool. Gas Chromatographs, while supplying this data, can be prohibitive due to cost, complexity, and need for on site technicians. Tunable filter spectroscopy is a viable technology for the drilling environment that enables the measurement of compositional gas data at a much higher rate than is offered by a gas chromatograph. Instruments utilizing tunable filter spectroscopy can be used to replace traditional total gas detectors as well as gas chromatographs while remaining economical unmanned solutions.